



# Application of Nuclear Physics


## Frontier of gamma-ray spectroscopy

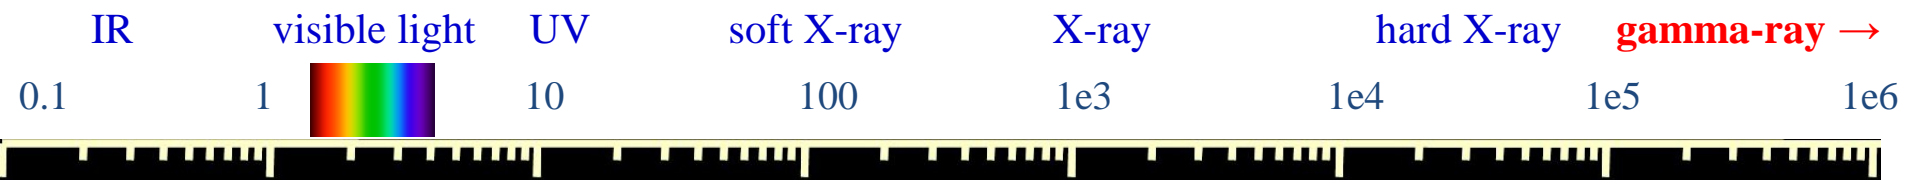



Photoelectric effect

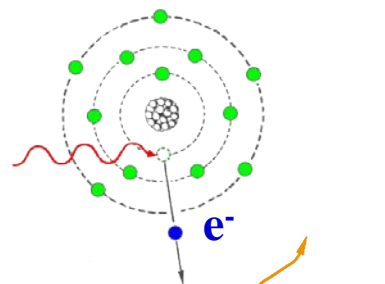

Compton scattering

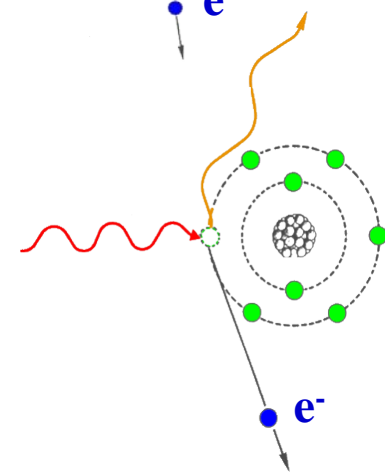

energy [eV]

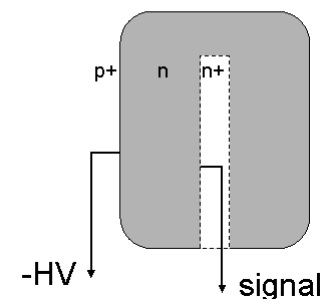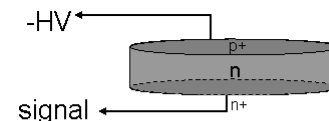


Germanium  
semi-conductor detectors

# Why imaging gamma-rays?

## ➤ High energy astrophysics

Correlate the detected photon to source object as known from more precise observations in other wavelength

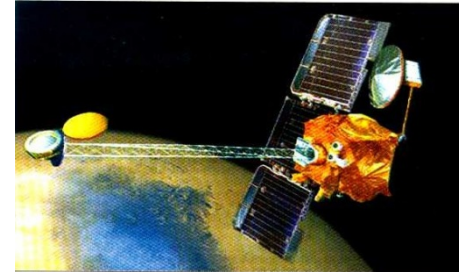


## ➤ Biomedical research

Precise localization of radioactive tracers in the body

Cancer diagnosis

Molecular targeted radiation therapy

Monitor changes in the tracer distribution → dynamic studies

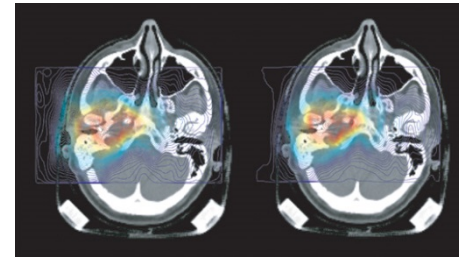

## ➤ National security

Nuclear non-proliferation / nuclear counter terrorism

Contraband detection

Stockpile stewardship

Nuclear waste monitoring and management

## ➤ Industrial non-destructive assessments


Determination of the material density distribution between the source and detector



# Application of Nuclear Physics

- ❖ First X-ray image by Wilhelm Conrad Roentgen (1895)

Standard X-ray imaging

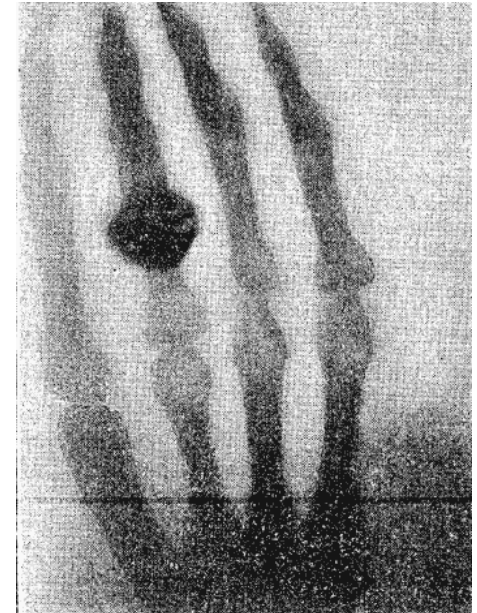

Absorption of X-rays by bones and transmission through soft tissue produces image


- What if we want a 3D image?
- What if we want detailed information on organs, bones and muscles etc?

Nobel Prize 1901

# Tomographic Imaging



PET

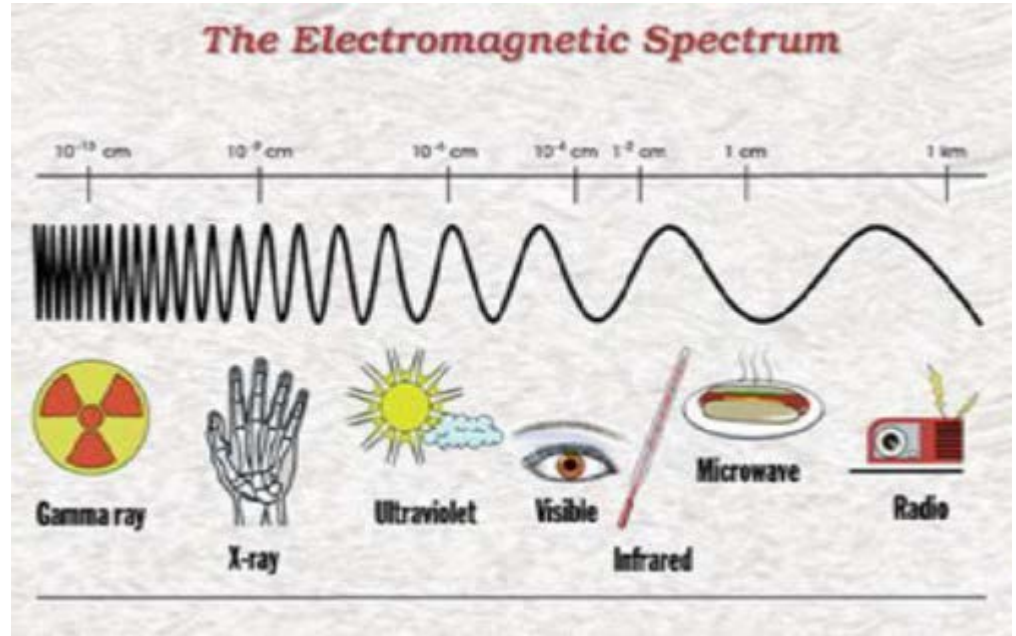

SPEC



CT



OPTICAL




MRI

# Computed Tomography

- ❖ CT scanning (originally known as CAT)
- ❖ X-rays taken at a range of angles around the patient
- ❖ Generation of 3D images

Radiation detector

X-ray source


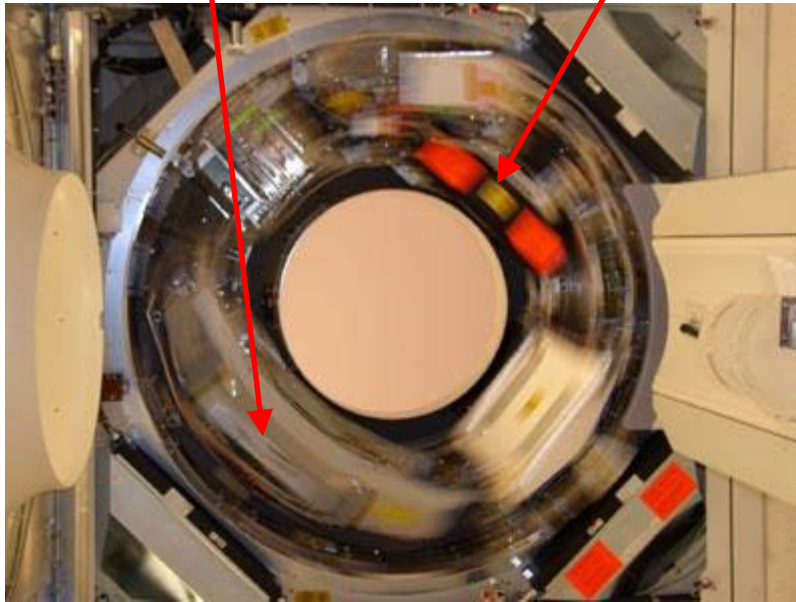


Standard CT-system



# Positron Emission Tomography


$^{11}\text{C}$

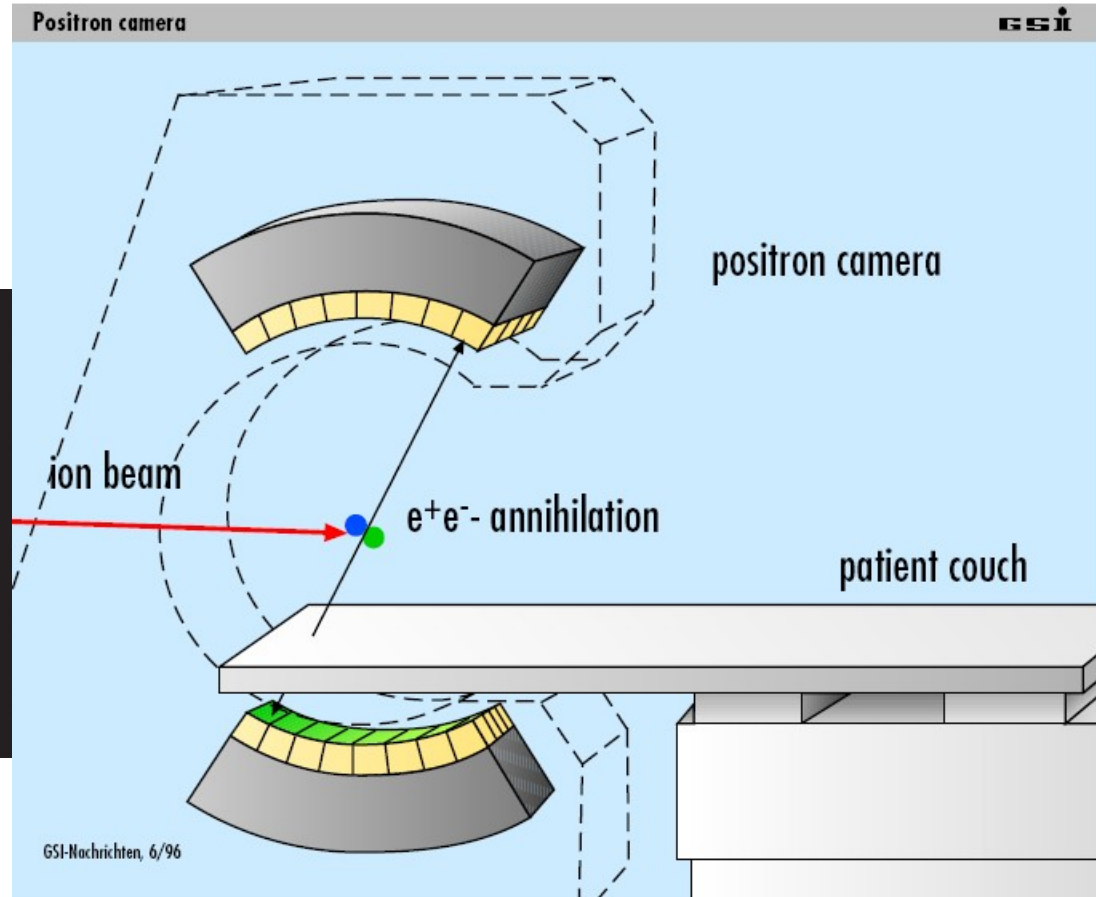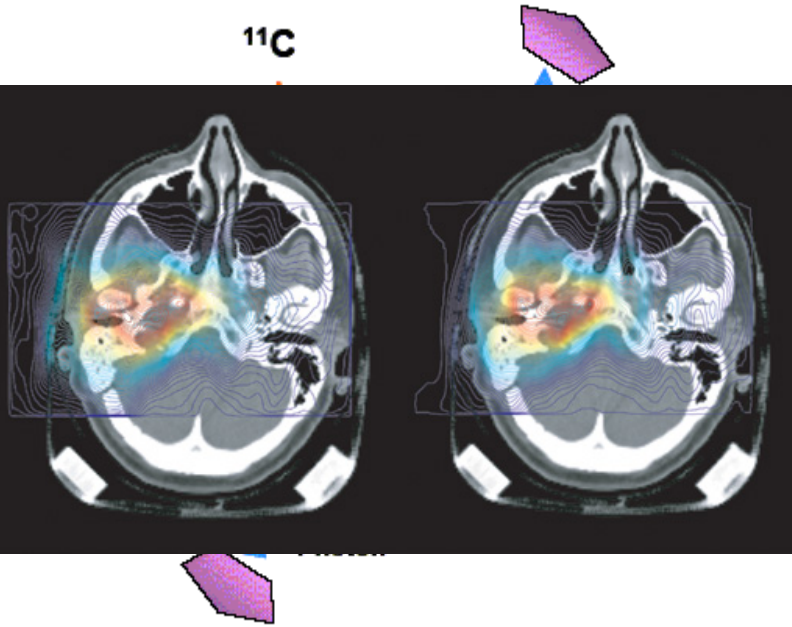

# Positron emission tomography




# Single Photon Emission Computed Tomography

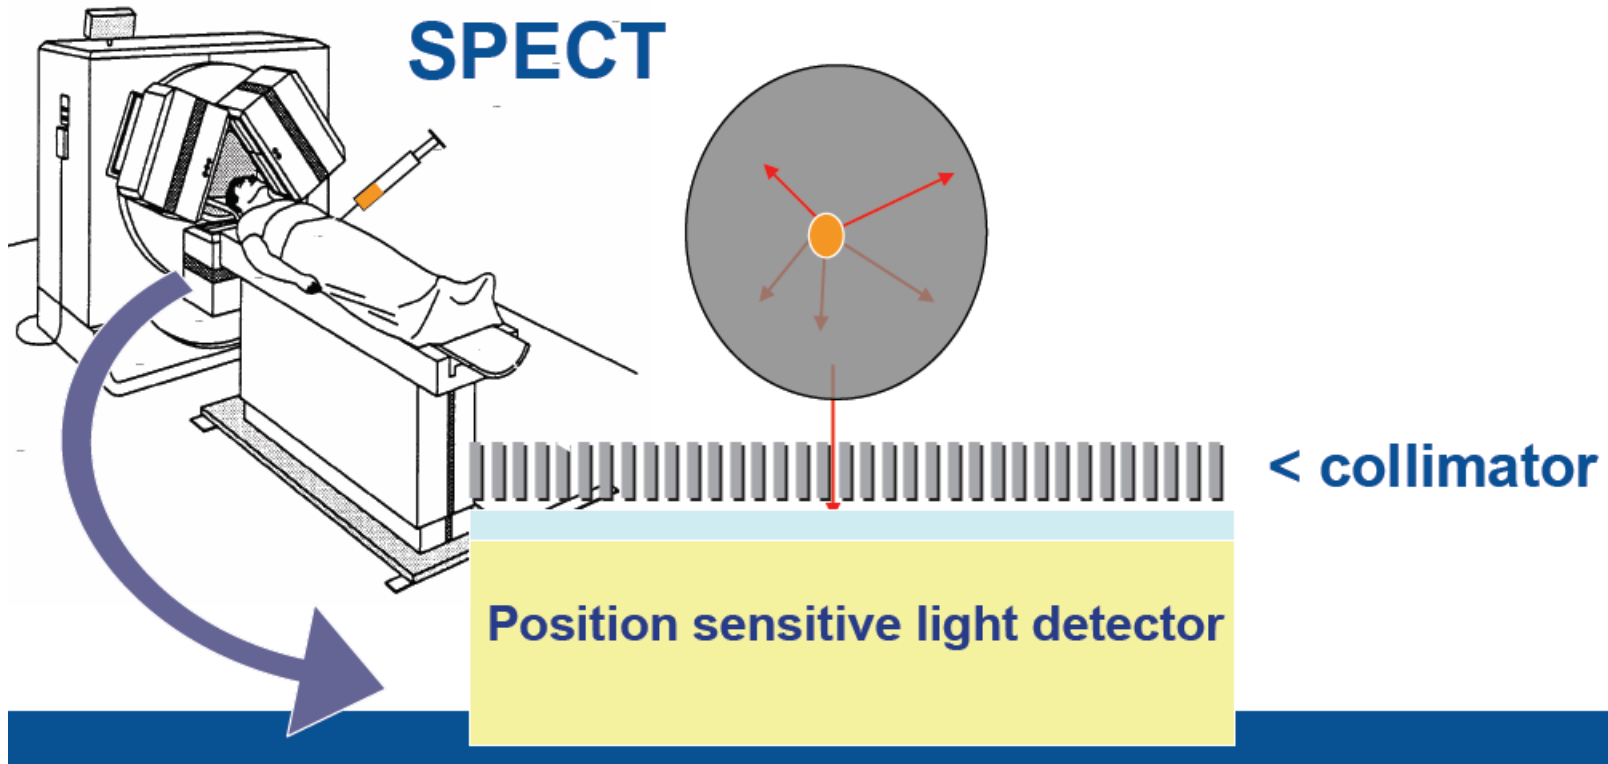


- ❖ Most commonly used tracer in SPECT is  $^{99}\text{Tc}^m$ , 140 keV a pure single photon emitter  $T_{1/2} = 6.02$  h.
- ❖ Utilizes a gamma-ray camera rotated in small  $\sim 3^\circ$  steps around the patient.




# The motivation behind the project

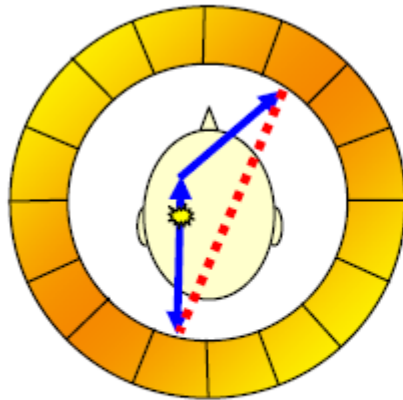

**Scattered  
Coincidence**

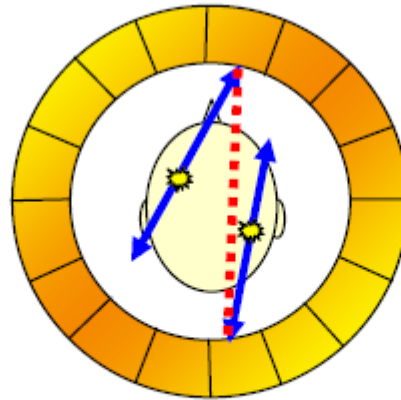

**Random  
Coincidence**

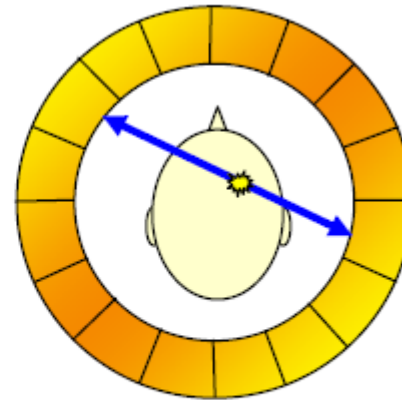

**True Coincidence**

- ❖ Existing technology relies on BGO scintillator technology
  - Limited position resolution
  - High patient dose requirement.
  - Poor energy resolution only accept photopeak events.
  - Will not function in large magnetic field
- ❖ SPECT applications utilizing Compton Camera techniques.

# Which $\gamma$ -ray camera to be used?


## Requirements:

- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

- Large FOV of  $\sim 20$  cm diam.
- Low spatial resolution 0.5-1 cm




www.siemens.de

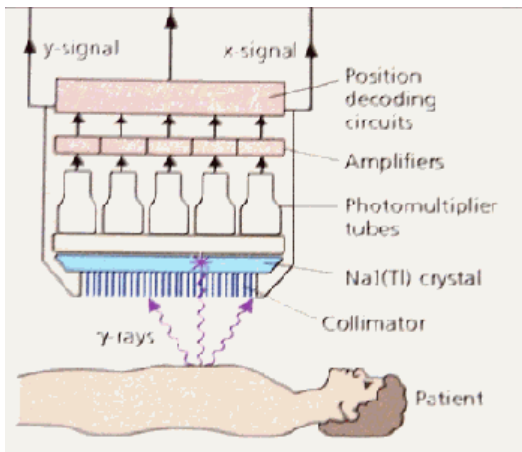

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm




Gem-imaging.com

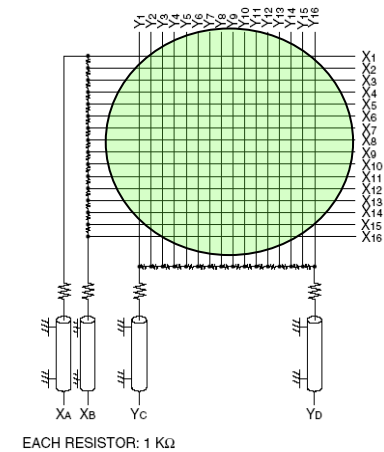

# Gamma Camera: Individual multi-anode readout


16 wires in X axis and 16 wires in Y axis

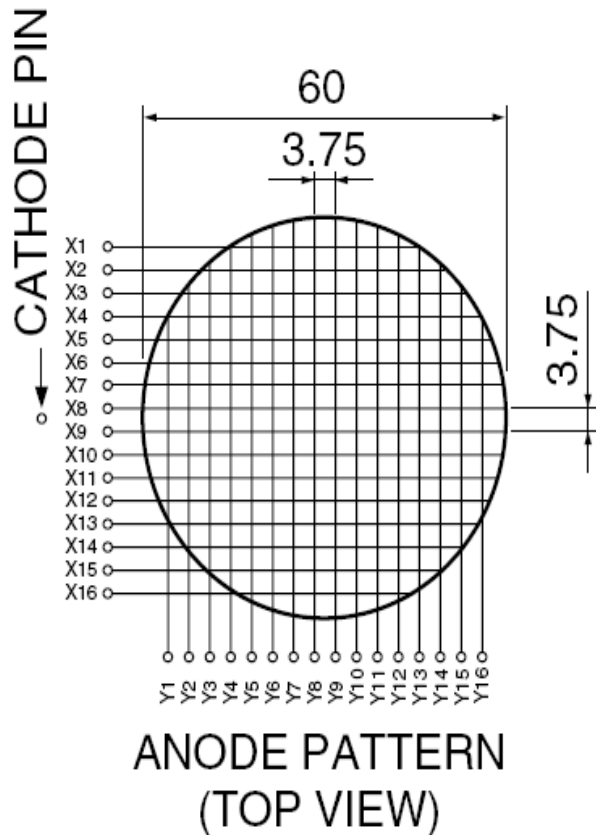

LYSO  
scintillator

$d = 76 \text{ mm}$   
 $t = 3 \text{ mm}$   
 $\rho = 7.4 \text{ g/cm}^3$

Hamamatsu R2486 PSPMT

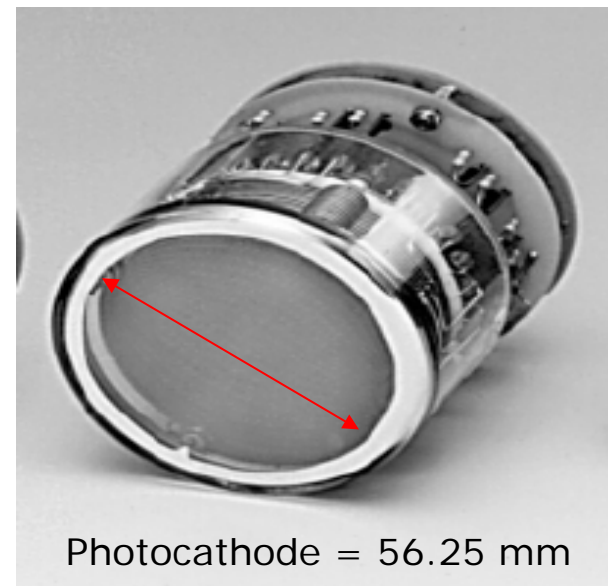


Photocathode = 56.25 mm

# Which $\gamma$ -ray camera to be used?

## Requirements:

- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

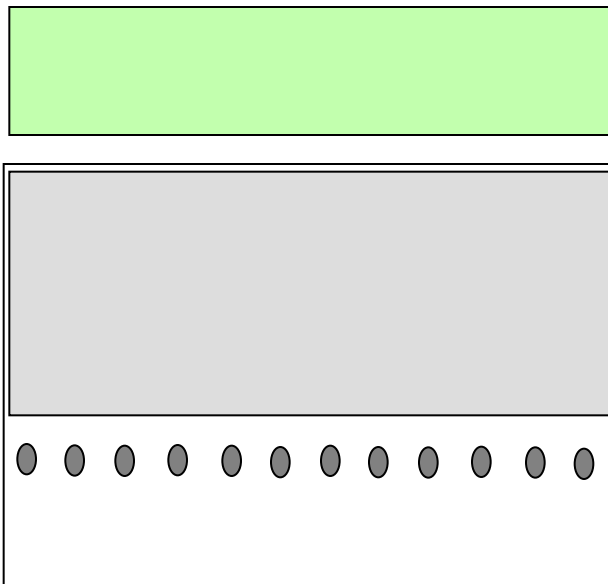

Scintillator


Position  
Sensitive

PMT

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm




Gem-imaging.com

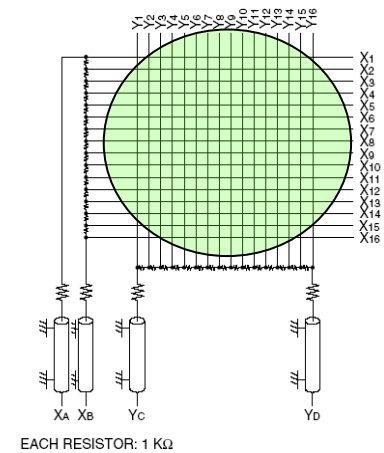


# Which $\gamma$ -ray camera to be used?

## Requirements:

- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

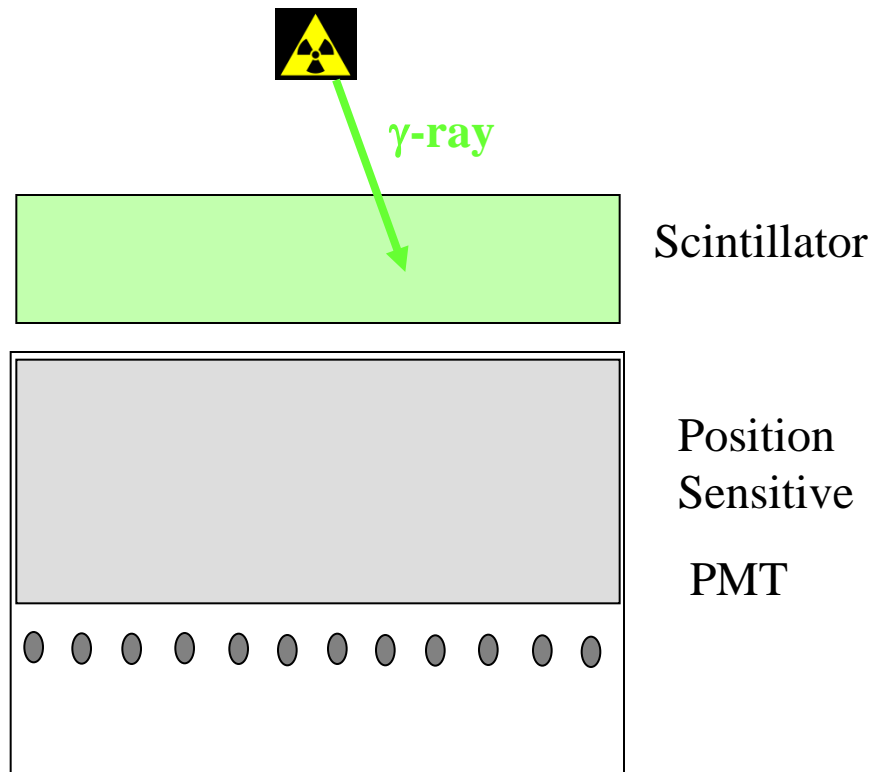

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm

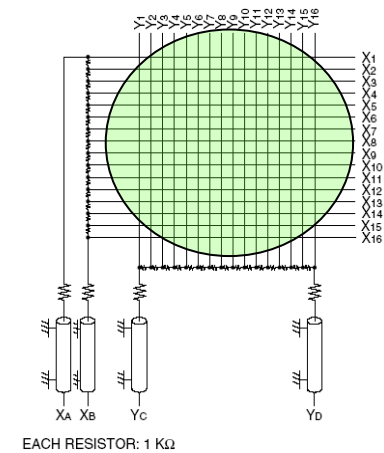


Gem-imaging.com

# Which $\gamma$ -ray camera to be used?

## Requirements:


- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

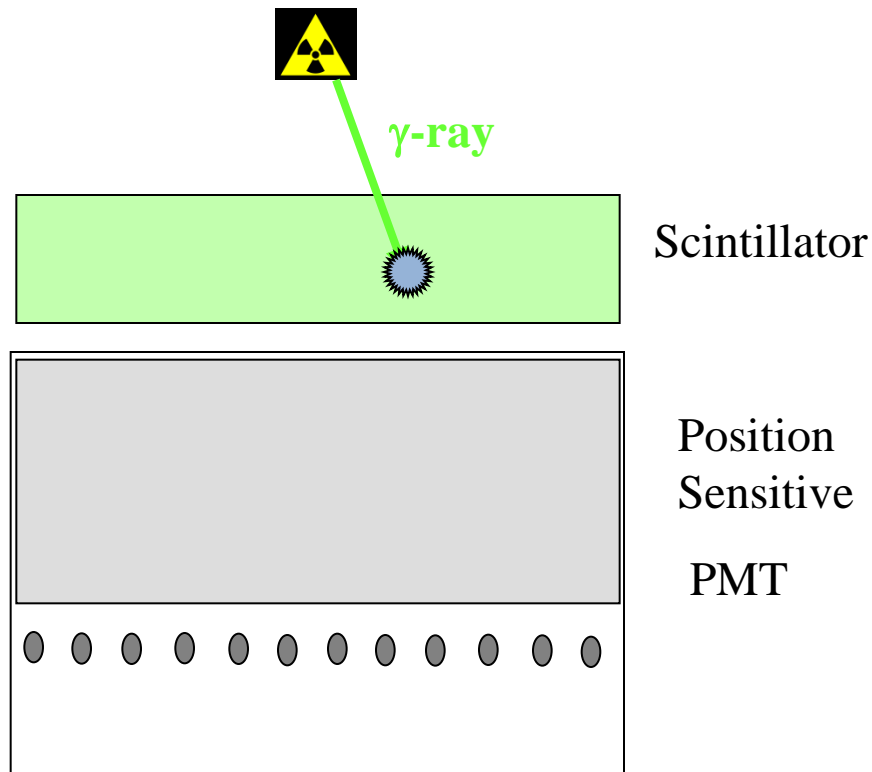

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm




Gem-imaging.com

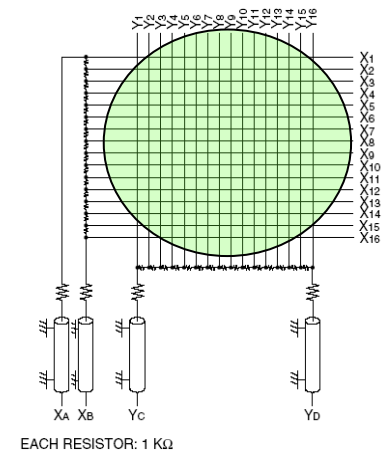

# Which $\gamma$ -ray camera to be used?

## Requirements:


- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

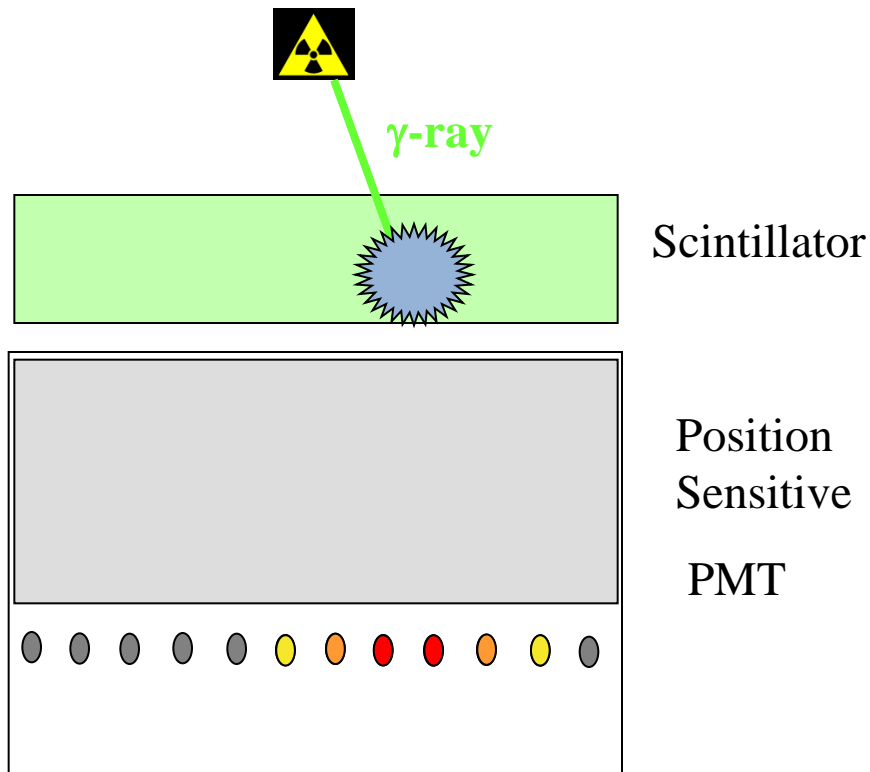

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm




Gem-imaging.com

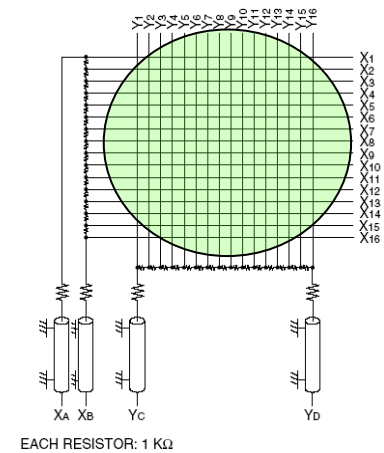

# Which $\gamma$ -ray camera to be used?

## Requirements:


- ❖ Excellent resolution  $\Delta x = 2$  mm
- ❖ Large field of view (FOV) =  $8 \times 9$  cm<sup>2</sup>

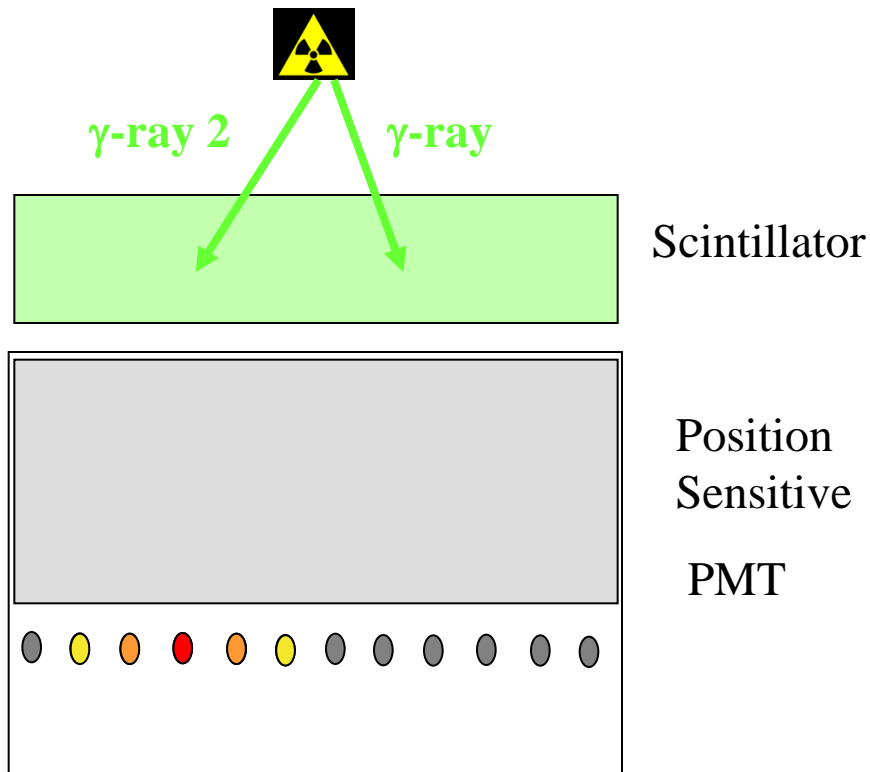

- Small FOV of 3-4 cm diam.
- High spatial resolution 2-3 mm




Gem-imaging.com

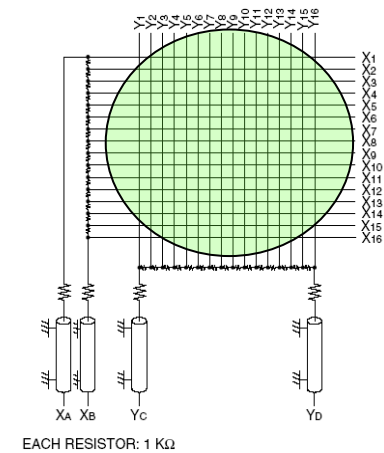





# HPGe detector – working principle

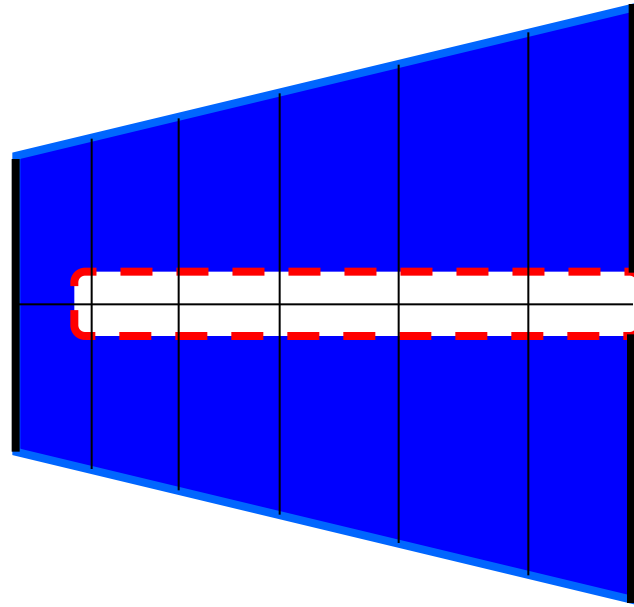



# HPGe detector – working principle

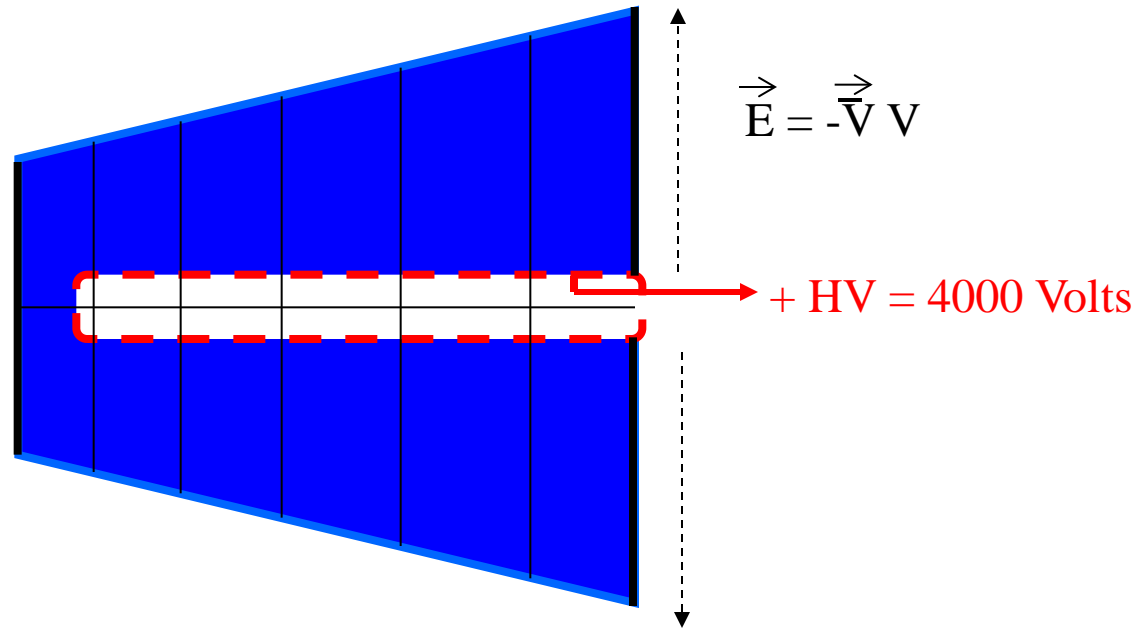



# HPGe detector – working principle

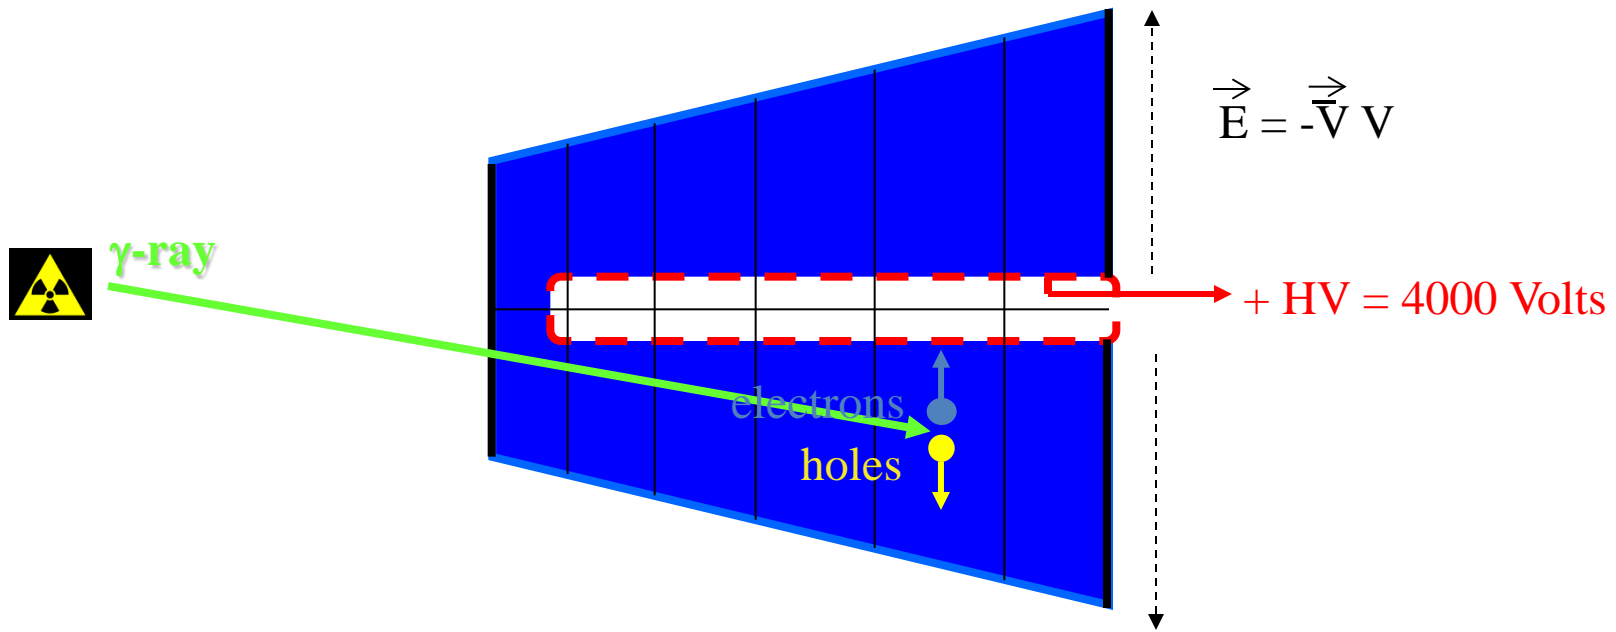



# HPGe detector – working principle

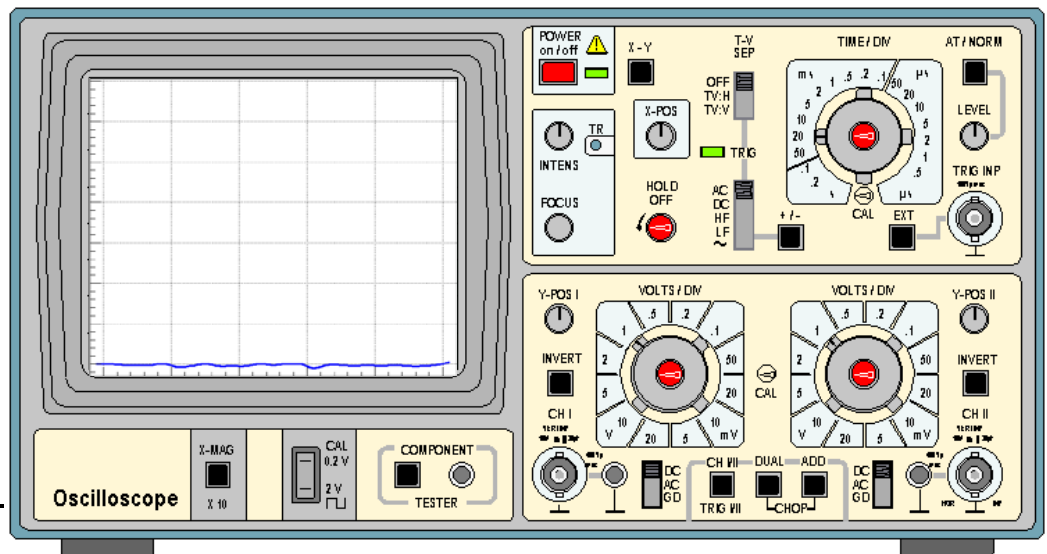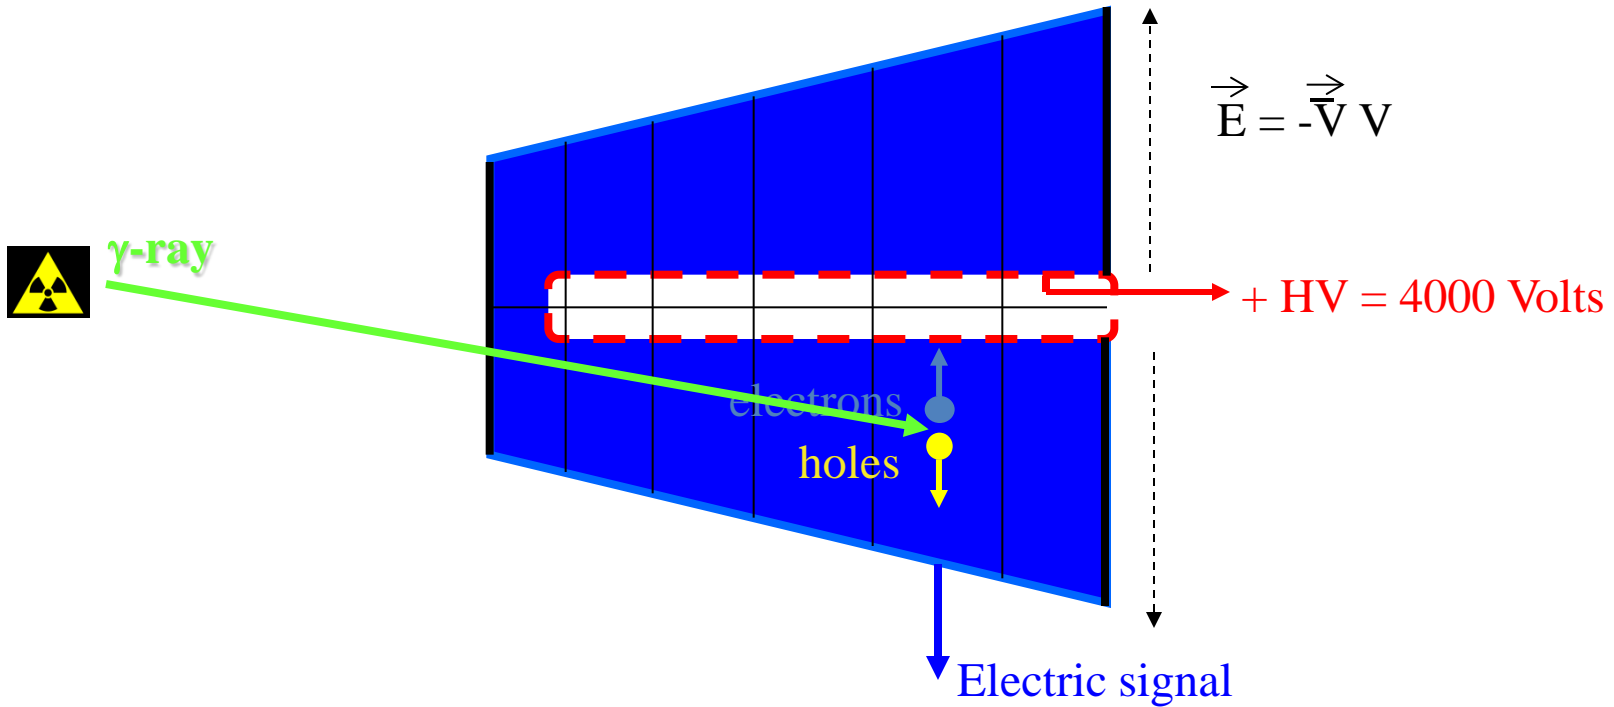



# HPGe detector – working principle

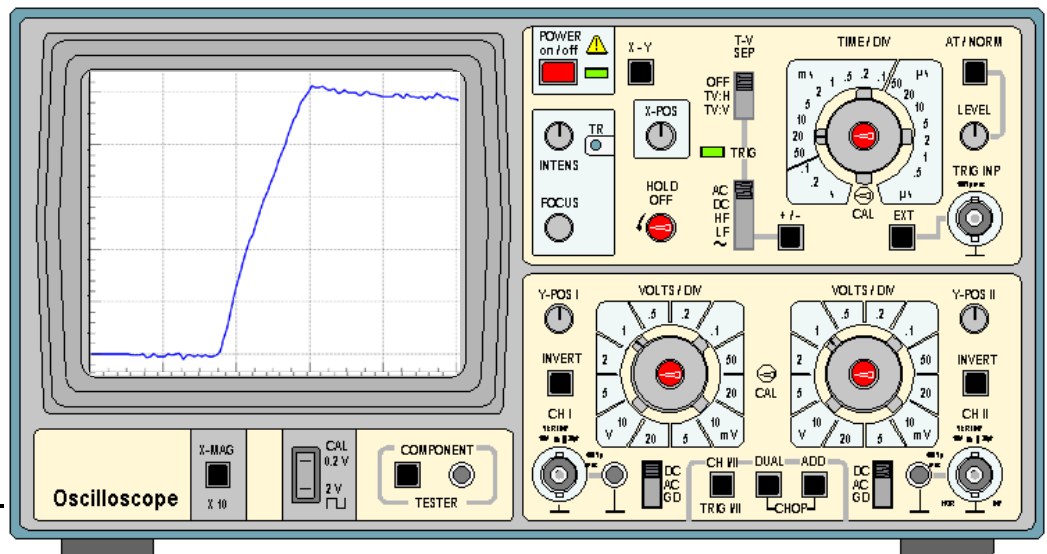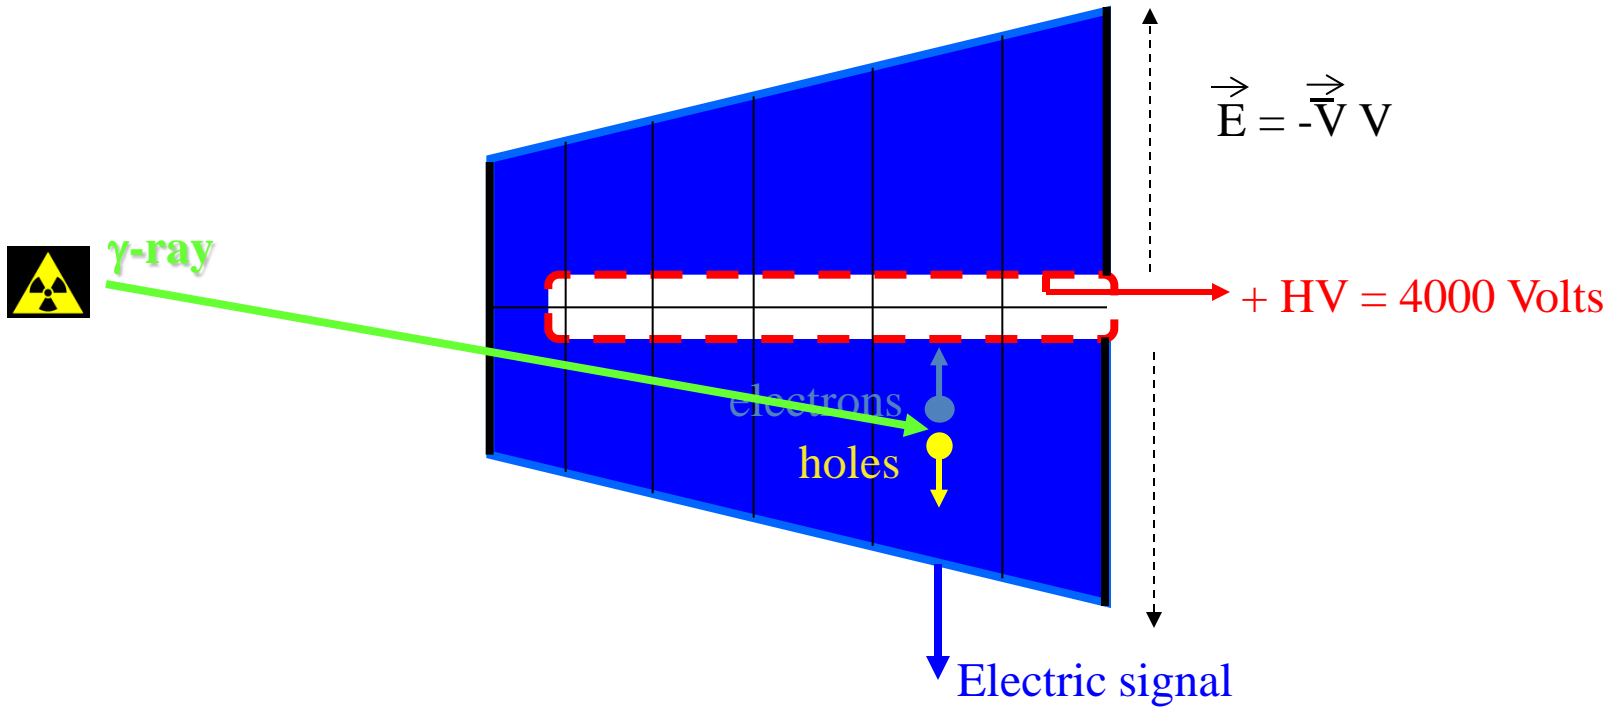



# HPGe detector – working principle

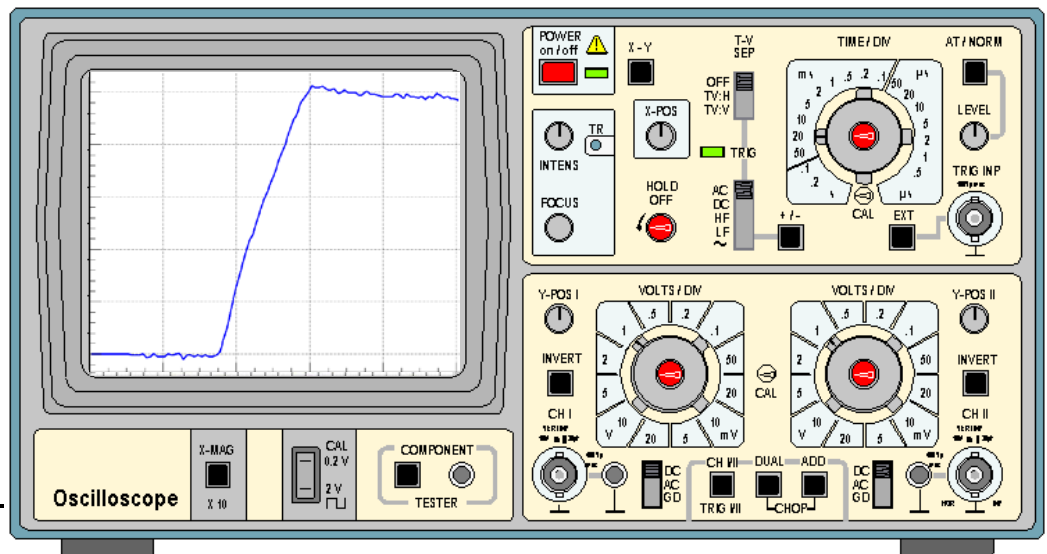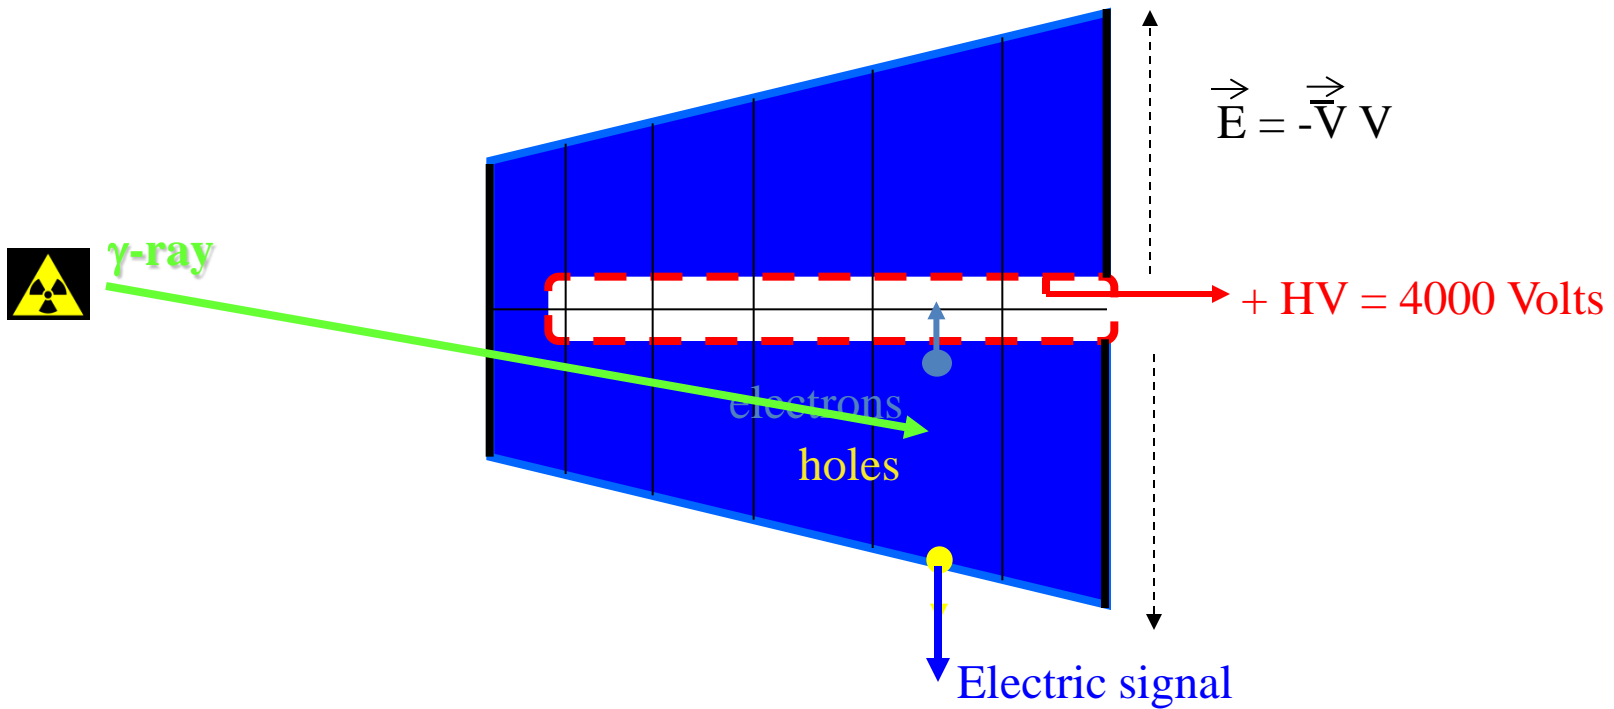

# HPGe detector – working principle

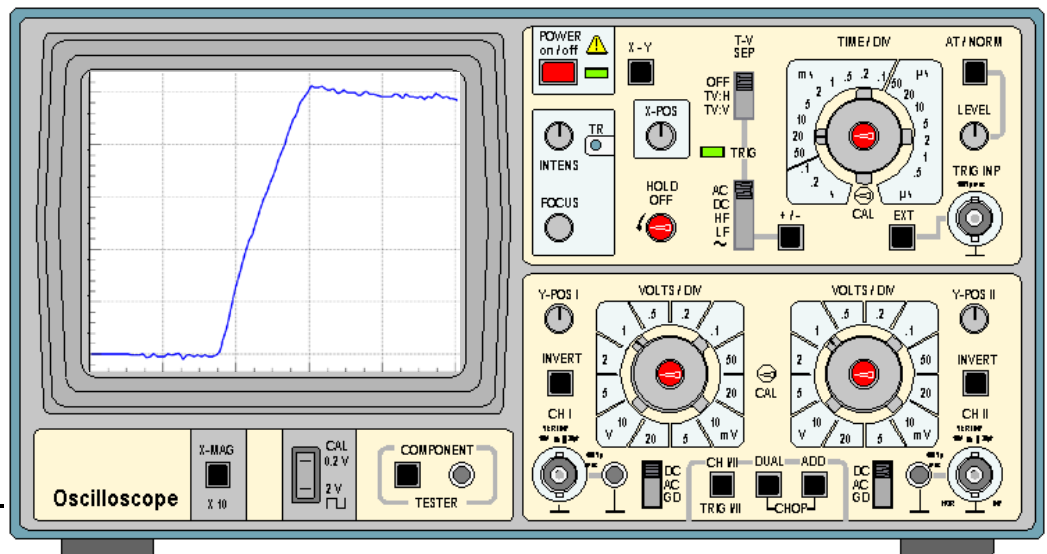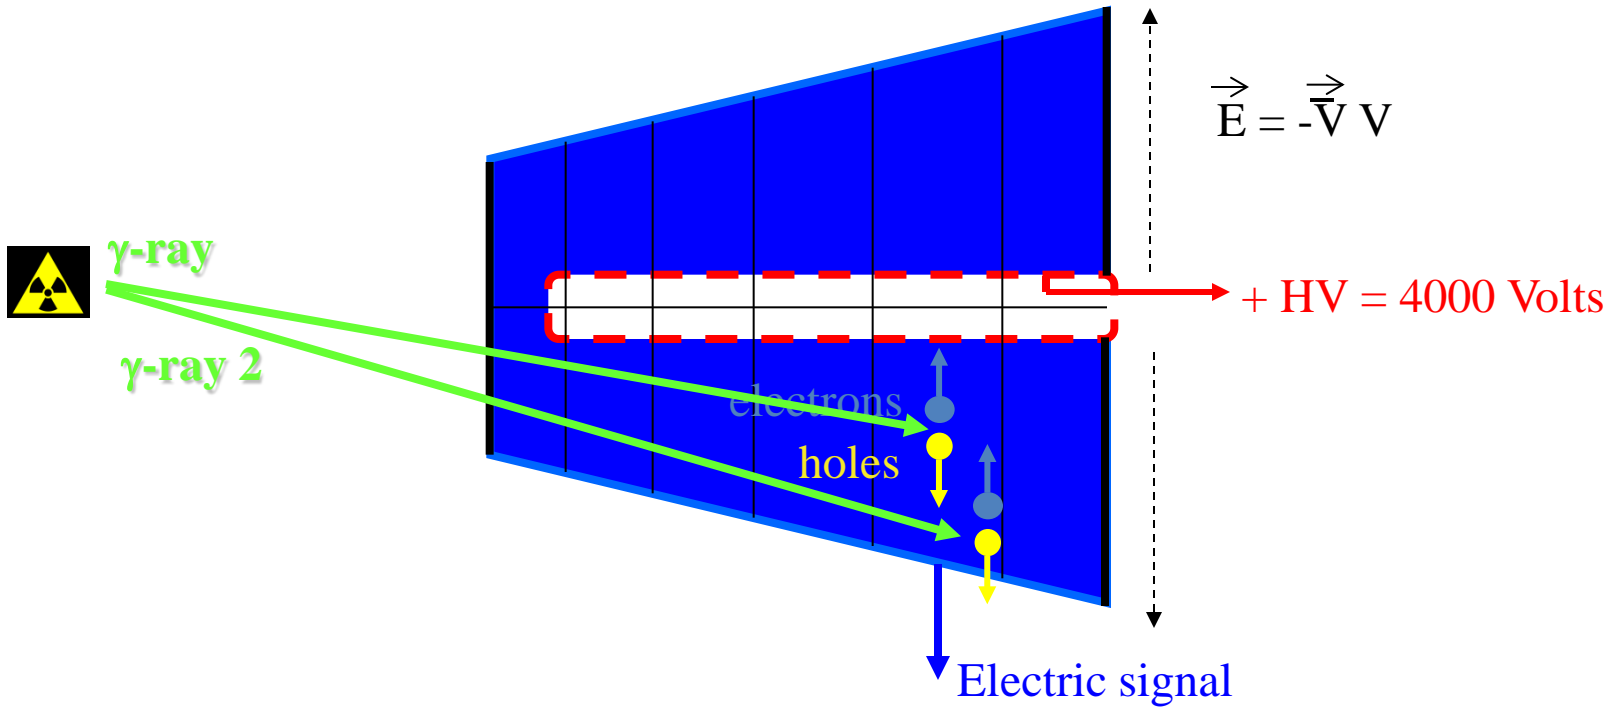

# HPGe detector – working principle

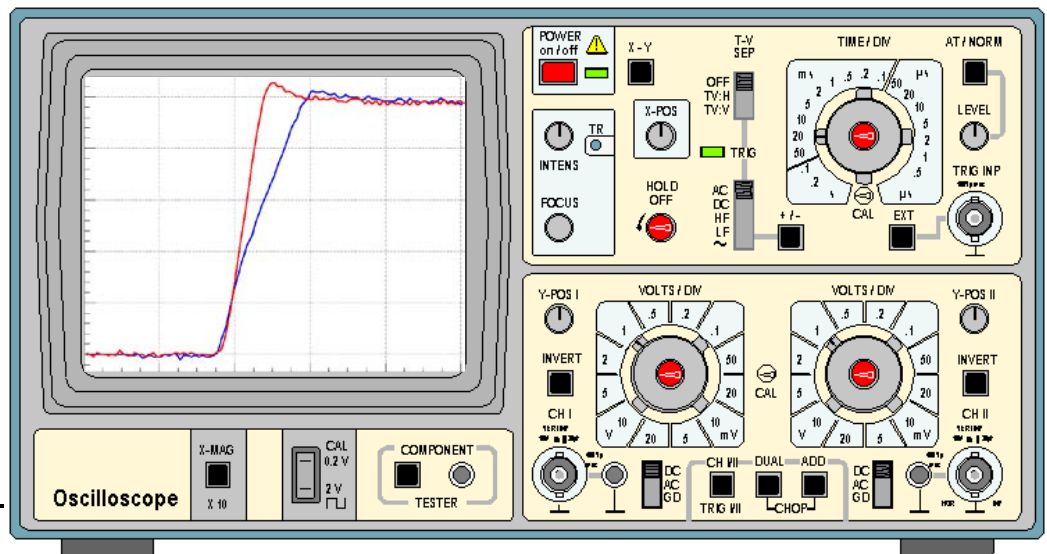
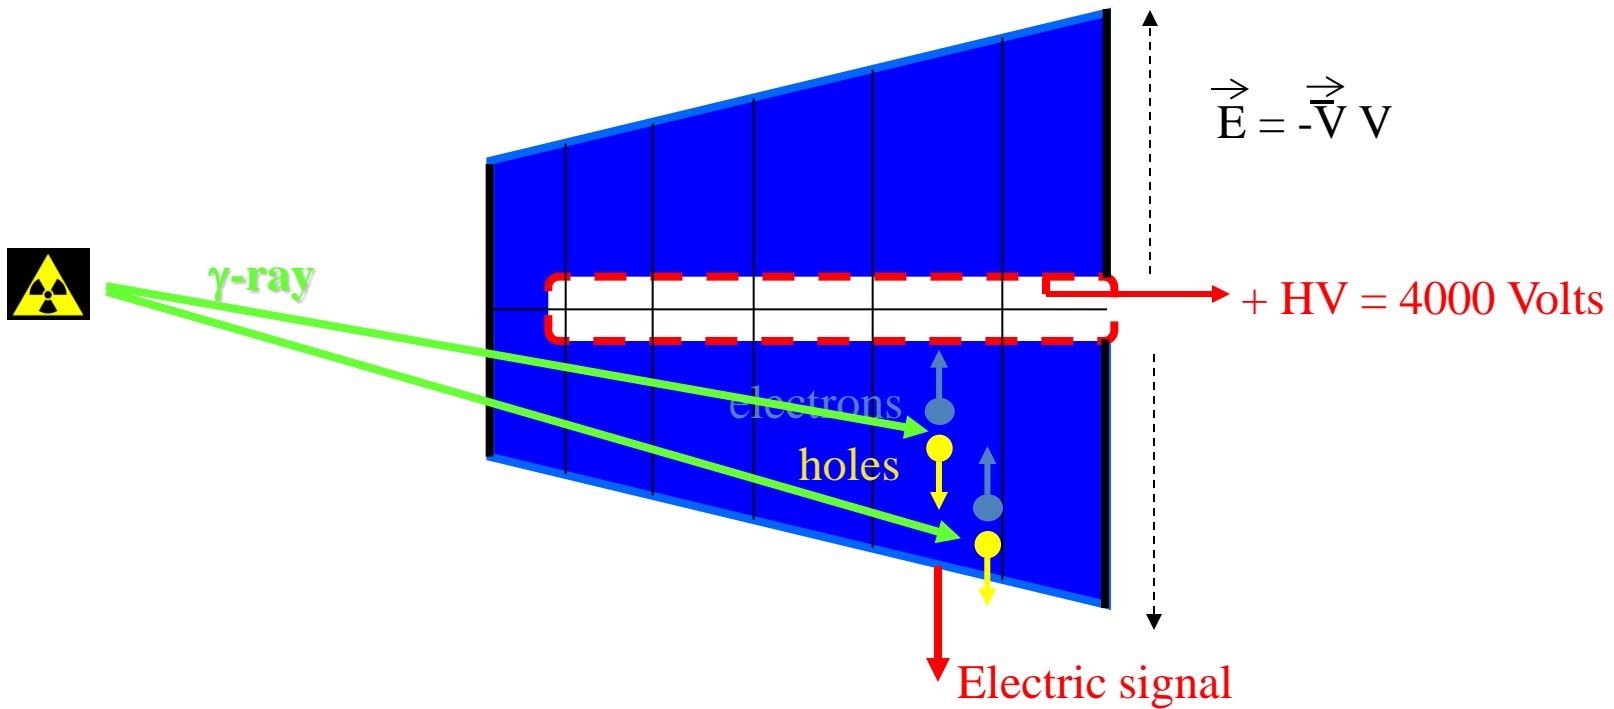




# Characterization of planar HPGe detector

Front view

Side view

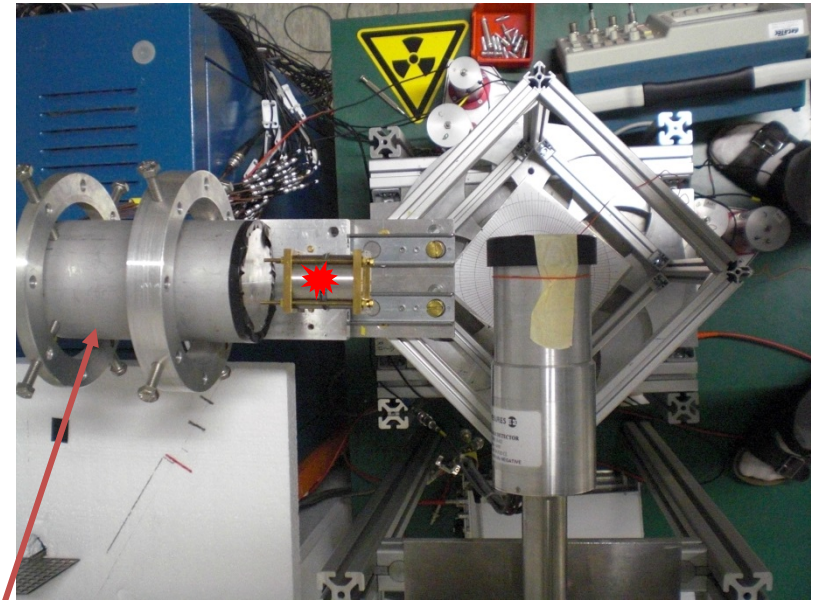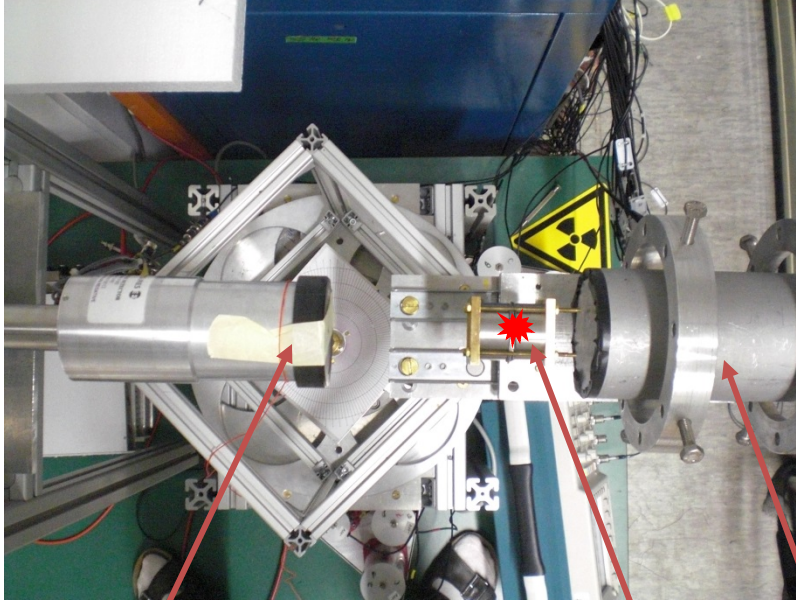

Planar Ge

$^{22}\text{Na}$






Position sensitive detector

$d = 4 \text{ cm}$

$t = 2 \text{ cm}$

# Planar HPGe detector scan

Intensity distribution for photopeak events

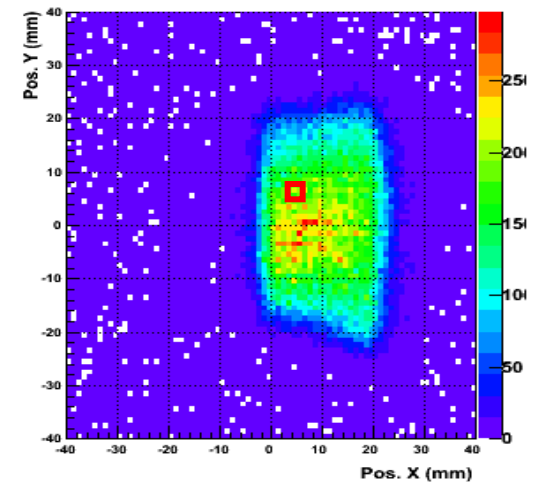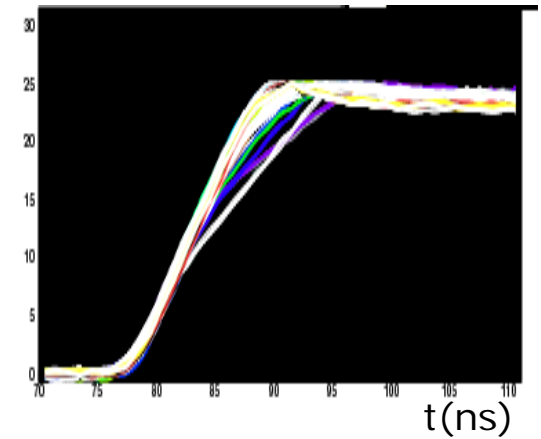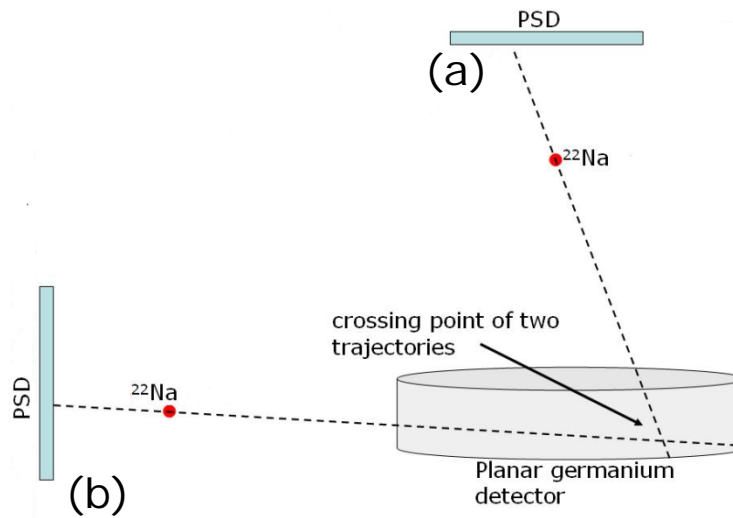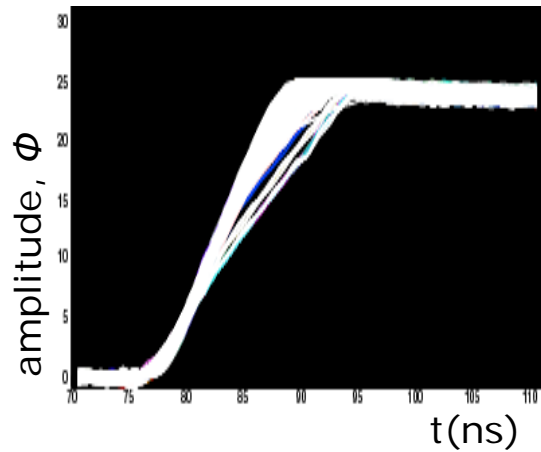
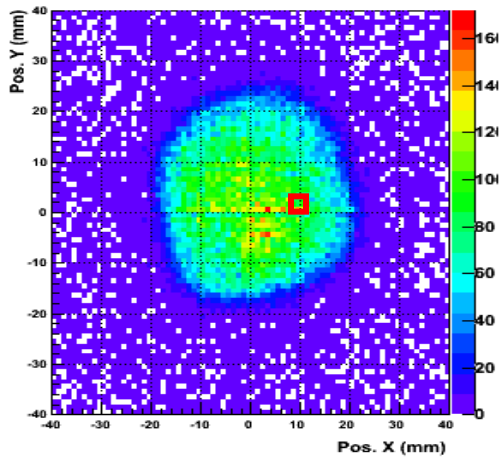


# Outlook




The GSI system uses conventional NIM and VME electronics, which makes it not easily portable, not easily scalable and rather expensive if one wants to build many of these devices.

However, this drawback could be overcome thanks to the increasing technology of electronics, e.g. a new acquisition system based on ASIC, FPGA, etc. technologies. This would also make the system more suitable for medical applications.

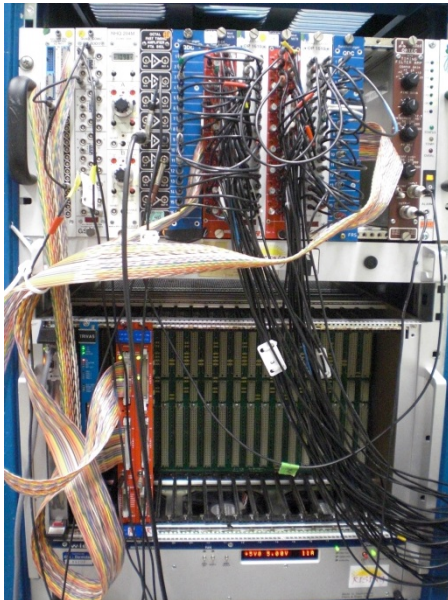




APV25 chip (from CERN CMS experiment)

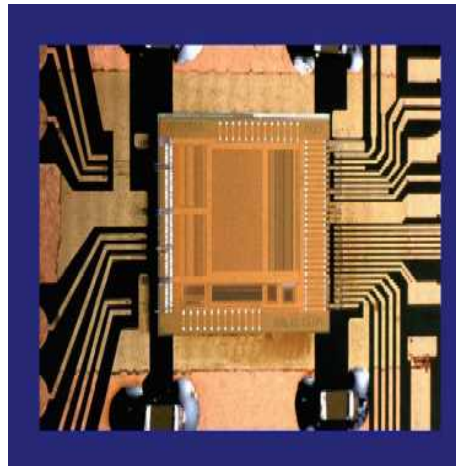

128-channel  
analogue  
pipeline chip

M.J. French et al., NIMA 466 (2001) 359

# Position Extraction in Planar Detectors

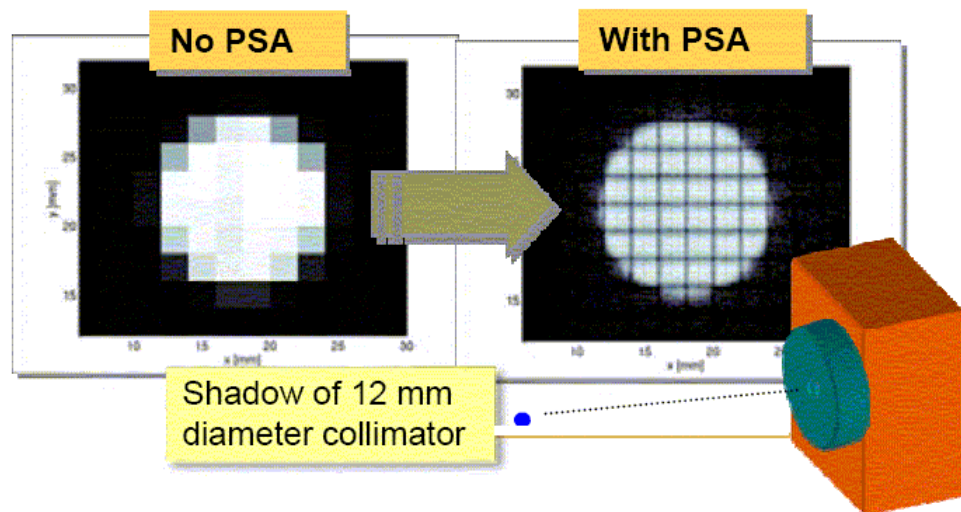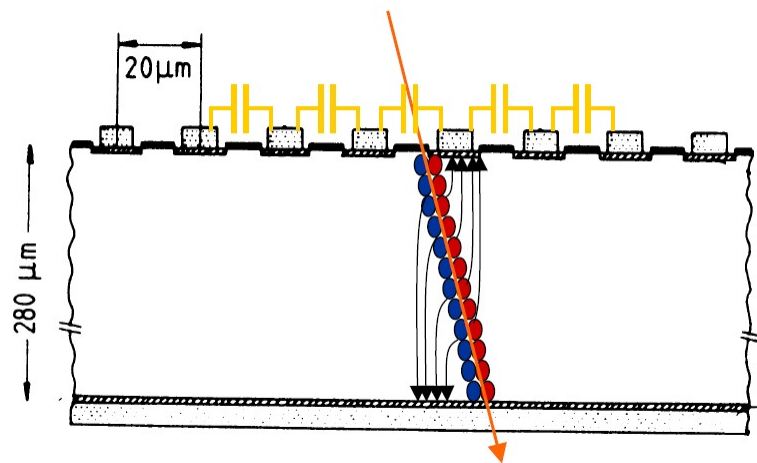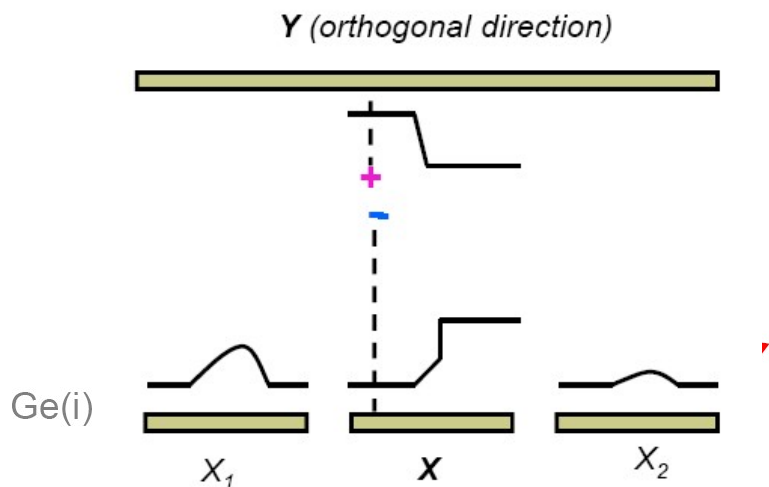


Position resolution of  $<0.5\text{mm}$  achieved at 122 keV in all three dimensions.

# Position Extraction in Planar Detectors


**LLNL - Double Sided Strip Detectors (DSSD) built of high-purity Ge and Li-drifted Si for gamma-ray imaging applications**

(Ethan Hull, LLNL, Paul Luke, LBNL, and Davor Protic, Research Center Juelich, Germany)

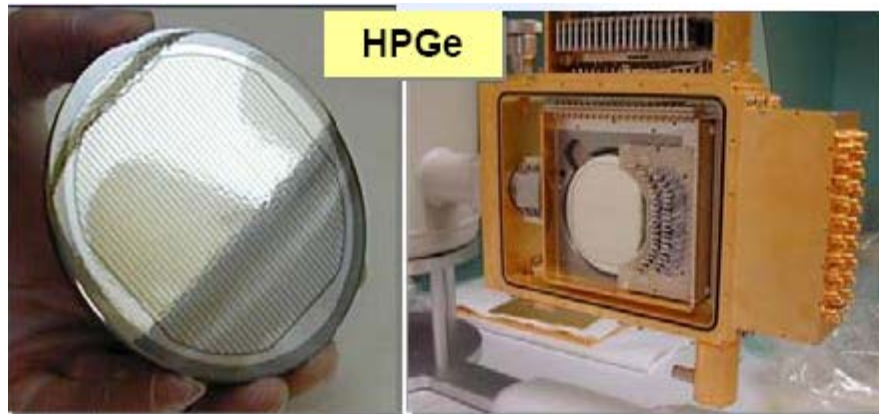

**HPGe**


2x38 strip DSSD HPGe detector with  
2 mm pitch and 11mm thickness

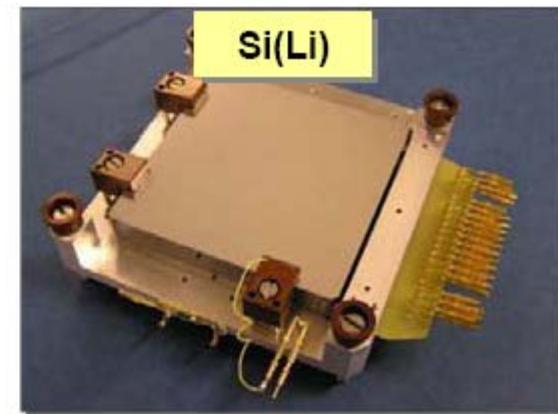


**Si(Li)**

2x32 strip DSSD Si(Li) detector with  
2 mm pitch and 10mm thickness

# Gamma-Ray Imaging

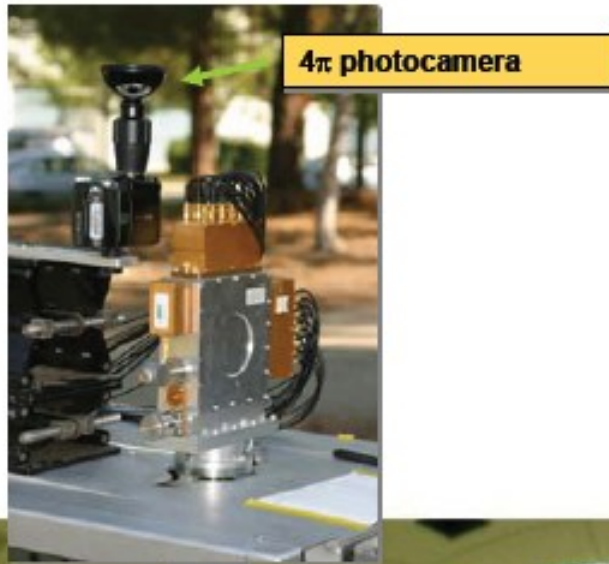

Gamma-ray imagers are detectors that separate radioactive objects from local background.

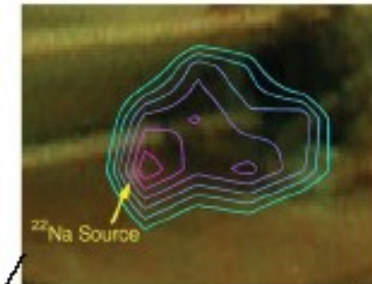

Conventional detectors accept gamma-rays from all directions and can be overwhelmed by local backgrounds.